

Calibration Studies and the Investigation of Track Segments within Showers with an Imaging Hadronic Calorimeter

Shaojun Lu, on behalf of the CALICE Collaboration

Max-Planck-Institute for Physics, and Excellence Cluster Universe, Munich, Germany

Abstract—The CALICE collaboration has constructed a highly granular hadronic sampling calorimeter prototype with small scintillator tiles individually read out by silicon photomultipliers (SiPM) to evaluate technologies for the ILC. The imaging capability of the detector allows detailed studies of the substructure of hadronic events, such as the identification of minimum ionizing track segments within the hadronic shower. These track segments are of high quality, so that they can be used for calibration, as an additional tool to Muons and to the built-in LED system used to monitor the SiPMs. These track segments also help to constrain hadronic shower models used in Geant4. Detailed MC studies with a realistic model of an ILC detector were performed to study the calibration requirements of a complete calorimeter system. The calibration strategy was tested on real data by transporting calibration constants from a Fermilab beam test to data recorded at CERN under different conditions.

Keywords: AHCAL, SiPM, Track Segments, Calibration

1. The CALICE Detectors

The goal of the CALICE experimental program is to establish novel technologies for calorimetry in future collider experiments and to record electromagnetic and hadronic shower data with unprecedented three dimensional spatial resolution for the validation of simulation codes and for the test and development of reconstruction algorithms. Such highly granular calorimeters are necessary to achieve an unprecedented jet energy resolution at the International Linear Collider¹ using particle flow algorithms.² The CALICE analog hadron calorimeter (AHCAL) prototype is a 38 layers sampling calorimeter, which is built out of scintillator tiles with sizes ranging from $30 \times 30 \text{mm}^2$ in the core of the detector to $120 \times 120 \text{mm}^2$. The light in each scintillator cell is collected by a wavelength shifting fiber, which is coupled to a silicon photomultiplier (SiPM) SiPM. The SiPMs are produced by the MEPhi/PULSAR group.³ They have a photo-sensitive area of $1.1 \times 1.1 \text{mm}^2$

containing 1156 pixels with a size of $32 \times 32 \mu\text{m}^2$. In total, the calorimeter has 7608 channels. A built-in LED calibration system with UV LEDs, is coupled to each cell by clear fibers, and equipped with PIN diodes to monitor the LED light intensity. The performance of the AHCAL was validated with positrons at various energies. Good linearity and satisfactory agreement with simulation up to an energy of 50 GeV has been observed.⁴

2. Track segments in hadronic showers

The high granularity of the active layers in the hadronic calorimeter and the cell-by-cell readout gives the CALICE detectors unprecedented imaging capabilities. This is exploited to study the topology of hadronic events in detail. Track segments created by charged particles produced within the hadronic shower can be identified, provided the particles travel an appreciable distance before interacting again and are separated from other activity in the detector.

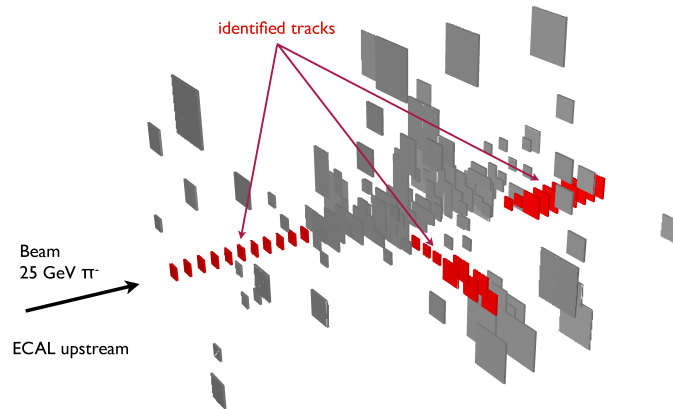


Fig. 1. Identification of minimum-ionizing track segments within hadronic showers.

Figure 1 demonstrated that three tracks were found within one 25 GeV π^- event. The properties of these tracks are sensitive to the substructure of the hadronic shower, and can thus serve as a powerful probe for hadronic shower models. The track segments identified in hadronic showers have a high quality, and are suitable for detector calibrations via the extraction

of the most probable value of the energy loss in each cell along the track. In the CALICE detector prototype, this technique was used to study the temperature dependence of the detector response.⁵

3. In-situ calibration strategy and requirements for an ILC calorimeter

Due to the underground location, the orientation of the detector layers, the power pulsing of the front end electronics, and due to the high granularity, calibrating a hadronic calorimeter with approximately 8 million channels at a future ILC detector is a significant challenge. Cosmic rays might not be sufficient for monitoring the energy scale in-situ. The track segments can be used for calibration purposes. A simulation study performed with a model of a complete ILC detector showed that a layer by layer calibration to a precision of better than 5% can be achieved with an integrated luminosity of 10 pb^{-1} at the Z^0 resonance.

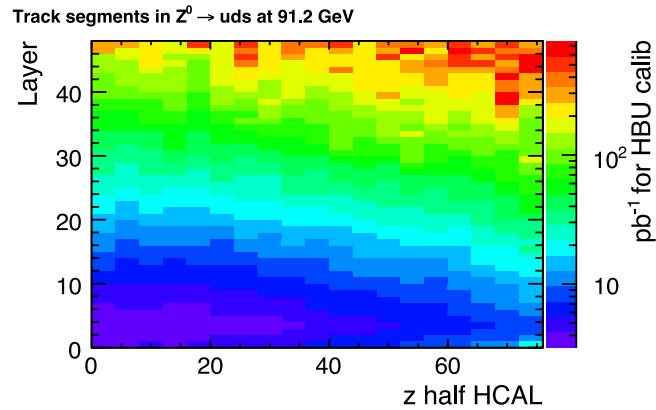


Fig. 2. Required luminosity for 1000 identified tracks in hadronic events per electronic unit HBU at Z^0 resonance running in the barrel AHCAL. One half of the AHCAL is shown, with the z coordinate of the interaction point at the lower left corner, z is measured here in units of tiles (3 cm).

Figure 2 shows the integrated luminosity required for the calibration of individual electronic subunits (144 cells), and illustrates the distribution of the number of found tracks within the calorimeter volume. At 500 GeV, this can be achieved with two weeks worth of data, for a calibration of the first 20 layers, one day is sufficient.

The single photon resolution of the SiPMs, together with an LED light system, can be used to perform a gain calibration of the photon sensor, and to monitor changes due to short term variations of environmental parameters. For a channel-by-channel intercalibration of the complete cell response, particles are necessary. Before installation, such a calibration can be performed in a beam, analogous to the muon calibration currently used for the CALICE detector system.⁶ Monitoring of long term variations, such as changes in the light yield of the scintillator have then to be performed in-situ. This can be achieved with track segments which are identified within the hadronic showers. To determine the requirement of calibration accuracy for the calorimeter of an ILC detector, a study has been performed for the scintillation-tile hadron calorimeter, based on full detector simulations. These studies demonstrate that spreads up to 10% in the layer to layer and cell by cell intercalibrations do not lead to a noticeable degradation of the overall performance in terms of the diijet energy resolution with particle flow algorithms.

4. Test of calibration strategy on real data

The calibration strategy was tested on real data by transporting calibration constants from a Fermilab beam test to data recorded at CERN. Two ways of transporting have been used, one based on the known temperature and voltage dependence of the SiPM response, and one based on measured changes in gain.

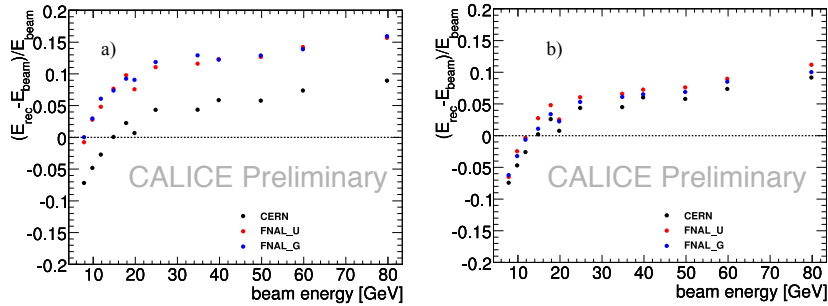


Fig. 3. a) Residual from linearity of reconstructed hadron showers fully contained in the AHCAL, in the range 8 to 80 GeV. b) Residual from linearity of reconstructed hadron showers fully contained in the AHCAL, in the range 8 to 80 GeV. adding the in-situ MIP stub correction layer-by-layer to each of the sample.

Figure 3 a shows a set of pion runs taken at CERN in the energy range 8 to 80 GeV were analyzed. The residual from linearity for the reference CERN calibration and for the two transported calibration sets were calculated. The hadronic energies calibrated with FNAL transported coefficients are approximately 5% higher than the reference CERN calibration sample. The two transport methods are in agreement with each other. The nonlinearity of the detector response is due to the requirement of full containment. After applying to all energy points an unique layer-by-layer correction derived from the identified track segments, a clear improvement in the agreement between different calibration methods is observed in figure 3 b. This demonstrates that an intercalibration of the detector modules in a beam before installation, and a layer-wise calibration with track segments after installation using regular physics data is sufficient to guarantee stable performance of the calorimeter at a future linear collider.

References

1. J. Brau, et al., *ILC Reference Design Report Volume 1 - Executive Summary*, arXiv:0712.1950 [physics.acc-ph], (2007)
2. M. A. Thomson, *Particle flow calorimetry and the PAndoraPFA Algorithm*, arXiv:0907.3577 [physics.ins-det], (2009)
3. G. Bondarenko et al., *Limited Geiger-mode microcell silicon photodiode: New results*, Nucl. Inst. Meth., vol. A442, pp. 187-192, (2000)
4. The CALICE Collaboration, *Electron data with the CALICE tile AHCAL prototype at the CERN test-beam*, CALICE Analysis Note 014, (2008)
5. F. Simon, *Track Segments in Hadronic Showers: Calibration Possibilities for a High Granular HCAL*, arXiv:0902.1879 [physics.ins-det], (2009)
6. F. Simon, *Calibration of a Highly Granular Hadronic Calorimeter with SiPM Readout*, arXiv:0811.2431 [physics.ins-det], (2008)